



Steelcase®
HEALTH


Sonata™ - Replacing a Drawer or Waste Bin Slide-Out on an Island or Nurse Servers

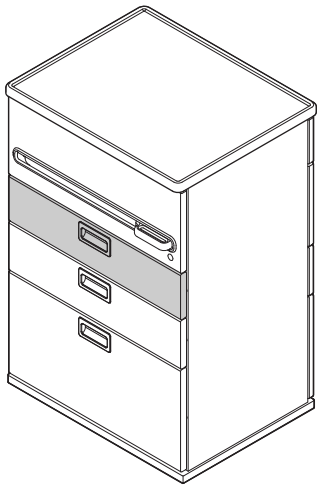

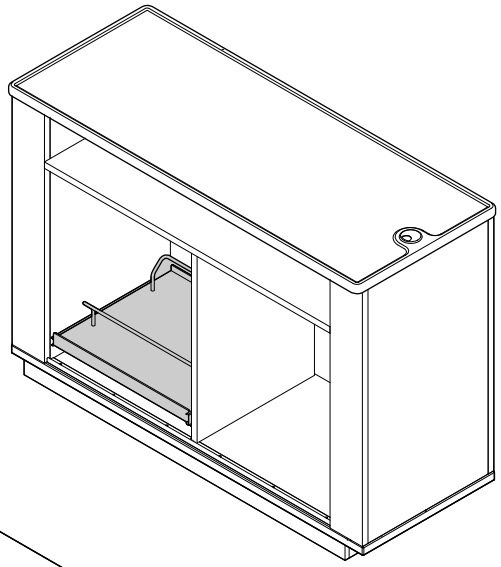

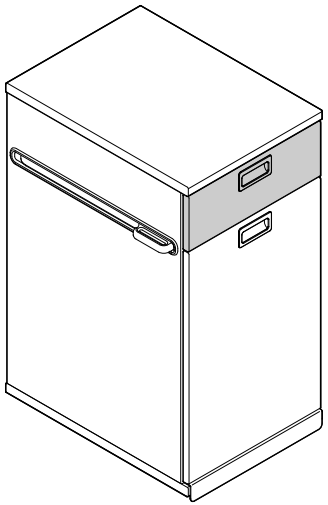





If you have a problem, question, or request, call your local dealer, or Steelcase Line 1 at **888.STEELCASE** (888.783.3522) for immediate action by people who want to help you.

(Outside the U.S.A., Canada, Mexico, Puerto Rico, and the U.S. Virgin Islands, call: 1.616.247.2500)
Or visit our website: www.steelcase.com

© 2014 Steelcase Inc.
Grand Rapids, MI 49501
U.S.A.

Printed in U.S.A.

Steelcase
HEALTH


Replacing a Waste Bin Slide-Out on an Island Module (shown) or Nurse Server with Trash


1. Pull waste bin slide-out outward.


2. Remove three (3) screws on each side of waste bin slide-out slide.

3. Push waste bin slide-out inward (3a) and then locate rectangular slot on the waste bin slide-out slide. Remove one (1) screw on each side of the waste bin slide-out slide (3b).

4. Remove waste bin slide-out and slides.

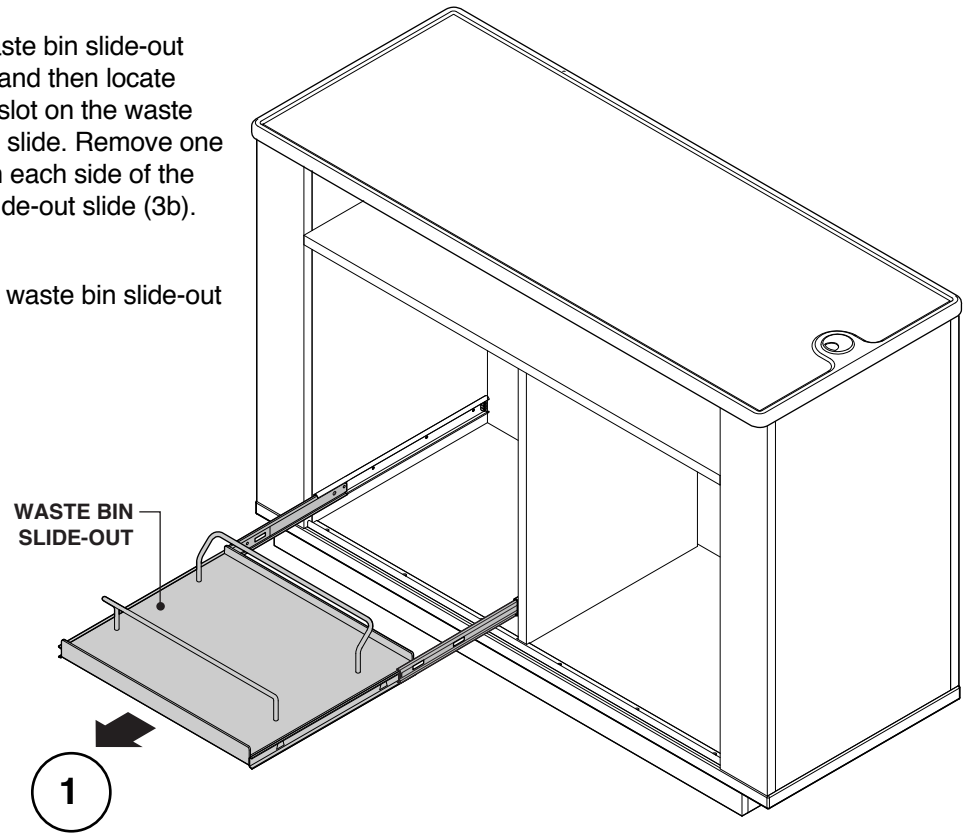


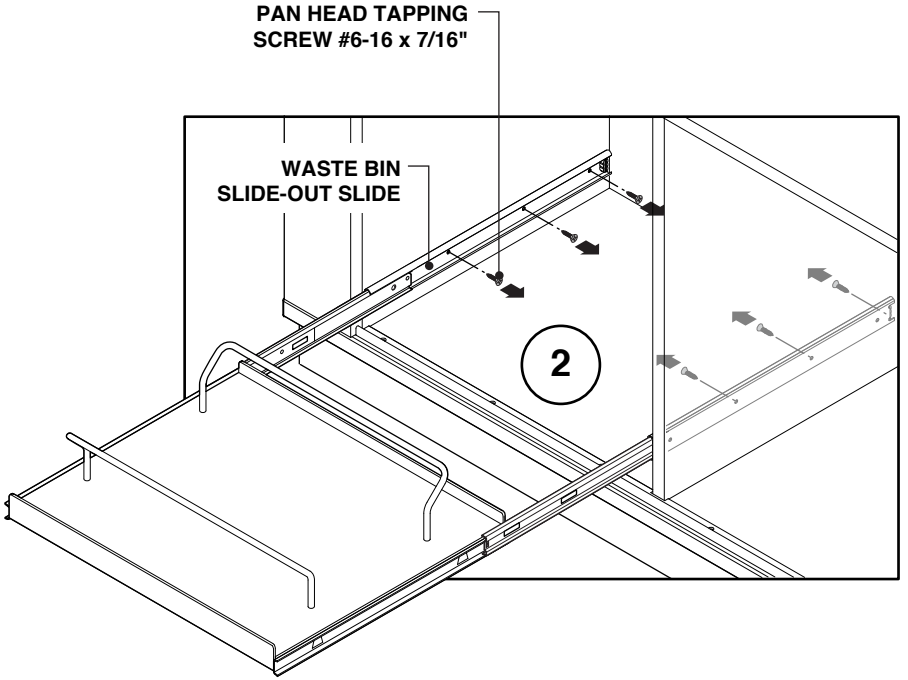

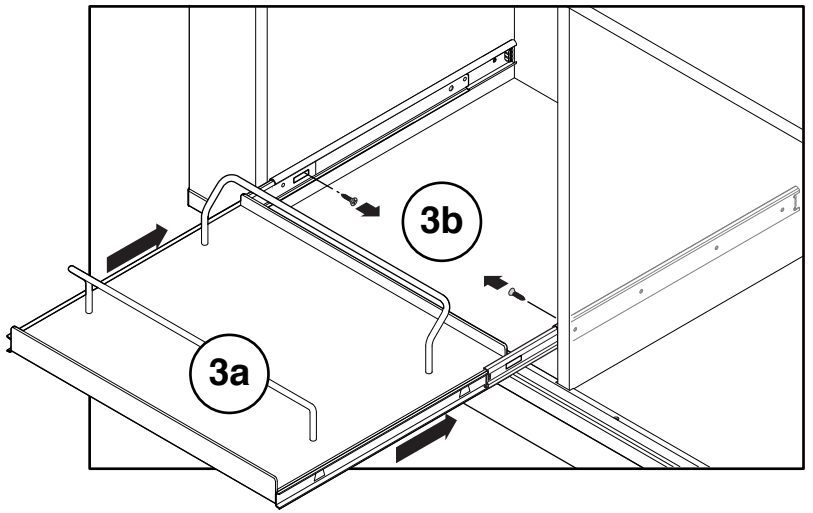

5. Remove the two slides by removing two (2) screws per slide.

6. Reverse steps 2 thru 5 to install a new waste bin slide-out and new slides.

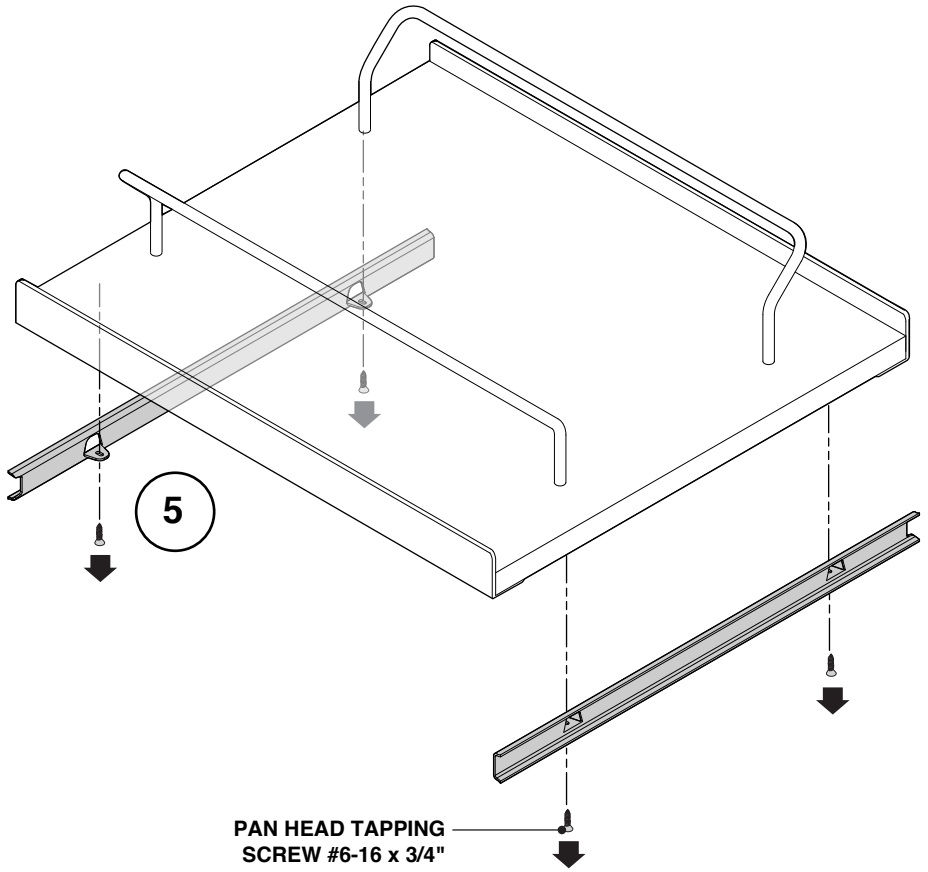

Steelcase
HEALTH


Replacing a Drawer on Nurse Server Modules

1. Pull drawer outward.

2. Push on tab on each side of the drawer.

3. Remove drawer.

4. Remove three (3) screws on each side of drawer slide mounting bracket.

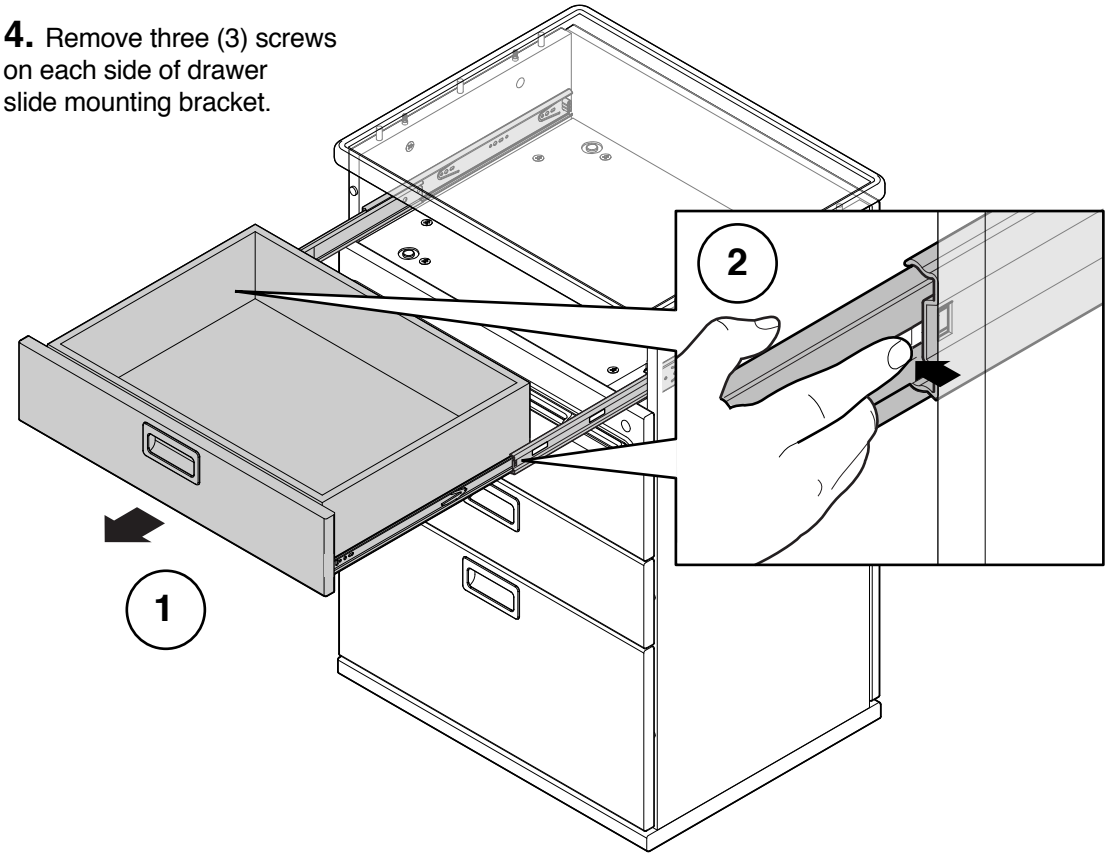

5. Push drawer slides inward (5a) and then locate rectangular slot on drawer slide. Remove one (1) screw on each side of drawer slide bracket (5b).

6. To install new drawer slides, reverse steps 4 and 5. To install drawer, reverse steps 1 thru 3.

